


# Brevetoxin (NSP) Plate, Detailed ELISA Procedure


## 1. Addition of Standards, Samples

Add 50  $\mu$ L of the standard solutions or samples into the wells of the test strips according to the working scheme given. We recommend using duplicates or triplicates.

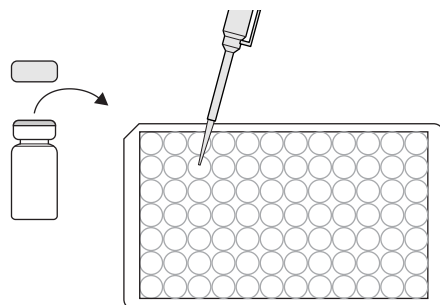


## 2. Addition of Reconstituted Enzyme Conjugate

Add 50  $\mu$ L of the reconstituted enzyme conjugate to the individual wells successively using a multi-channel pipette or a stepping pipette. Cover and mix for 30 seconds by rotating on benchtop. Incubate for 60 minutes at room temperature.

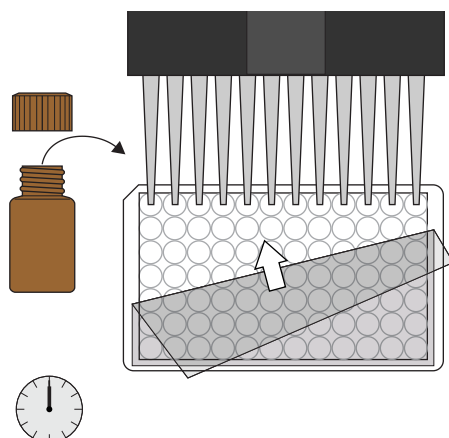


## 3. Washing of Plates

After incubation, remove the covering and vigorously shake the contents of the wells into a sink. Wash the strips three times with a multi-channel pipette or wash bottle using the diluted 1X washing buffer solution. Please use at least a volume of 250  $\mu$ L of washing buffer for each well and each washing step. Remaining buffer in the wells should be removed by patting the plate dry on a stack of paper towels.

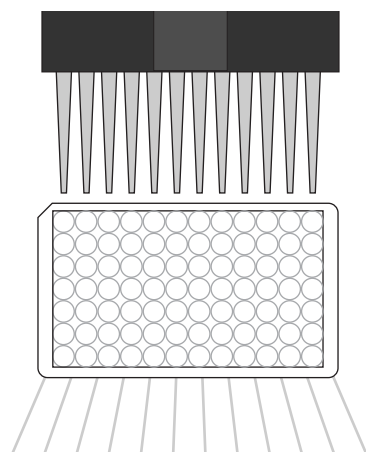


## 4. Addition of Substrate/Color Solution

Add 100  $\mu$ L of substrate/color solution to the individual wells successively using a multi-channel pipette or a stepping pipette. Cover the wells with parafilm or tape and mix the contents by moving the strip holder in a rapid circular motion on the benchtop. Be careful not to spill contents. Incubate the strips for 30 min at room temperature.

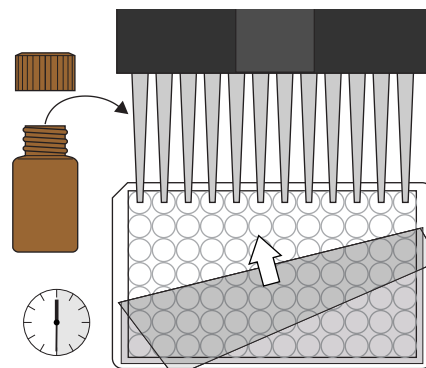


## 5. Addition of Stopping Solution

Add 100  $\mu$ L of stop solution to the wells in the same sequence as for the substrate solution using a multi-channel pipette or a stepping pipette.

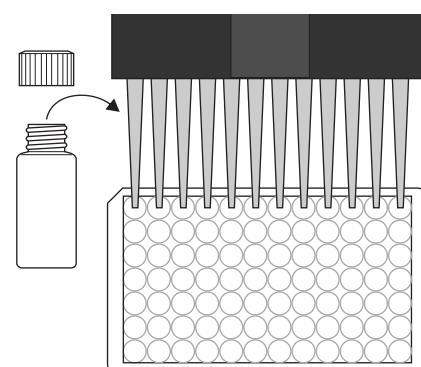

## 6. Measurement of Color

Read the absorbance at 450 nm using a microplate ELISA reader. Calculate results.

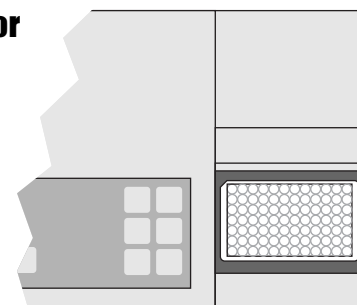


Eurofins Abraxis  
124 Railroad Drive, Warminster, PA 18974 USA  
Phone: 215-357-3911 Fax: 215-357-5232  
[www.abraxiskits.com](http://www.abraxiskits.com)  
Technical Support:  
[Support.ET.Warminster@eurofinsUS.com](mailto:Support.ET.Warminster@eurofinsUS.com)  
Ordering:  
[Info.ET.Warminster@eurofinsUS.com](mailto:Info.ET.Warminster@eurofinsUS.com)

# Brevetoxin (NSP) Plate, Concise ELISA Procedure


## 1. Addition of Standards, Samples

Add 50  $\mu$ L of standard solutions or samples.

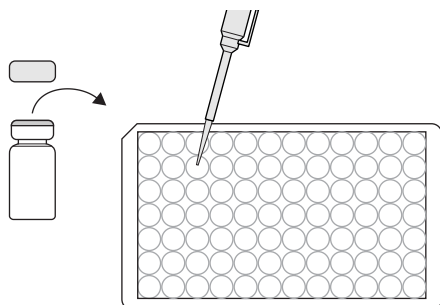


## 2. Addition of Reconstituted Enzyme Conjugate

Add 50  $\mu$ L of reconstituted enzyme conjugate. Cover and mix for 30 seconds by rotating on benchtop. Incubate for 60 minutes at room temperature.

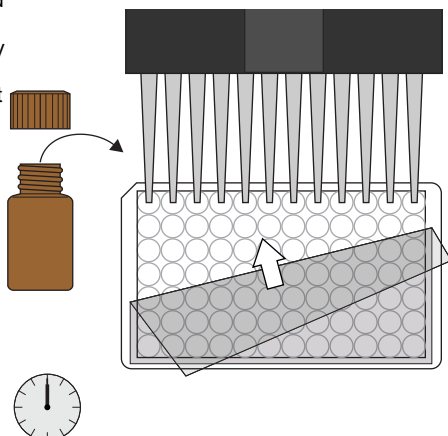


## 3. Washing of Plates

Wash the plates three times with 250  $\mu$ L of diluted 1X washing buffer.

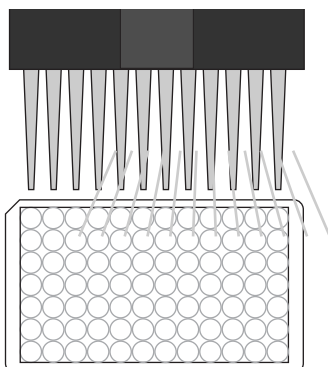


## 4. Addition of Substrate/Color Solution

Add 100  $\mu$ L of substrate/color solution. Incubate 30 minutes at room temperature and away from direct sunlight.

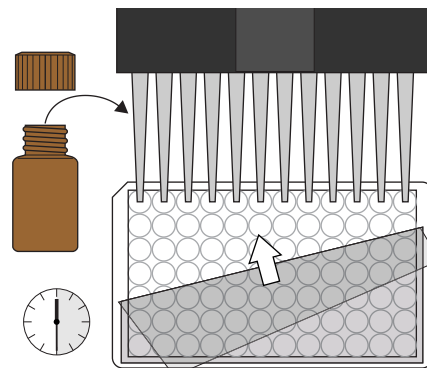


## 5. Addition of Stopping Solution

Add 100  $\mu$ L of stop solution.

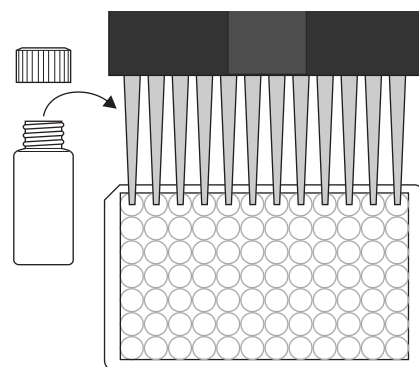

## 6. Measurement of Color

Measure color at 450 nm. Calculate results.

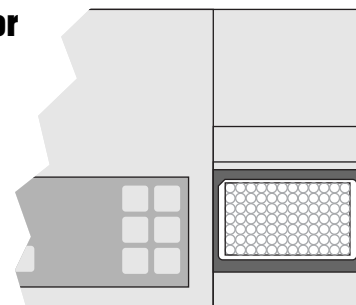

Eurofins Abraxis  
124 Railroad Drive, Warminster, PA 18974 USA  
Phone: 215-357-3911 Fax: 215-357-5232  
[www.abraxiskits.com](http://www.abraxiskits.com)  
Technical Support:  
[Support.ET.Warminster@eurofinsUS.com](mailto:Support.ET.Warminster@eurofinsUS.com)  
Ordering:  
[Info.ET.Warminster@eurofinsUS.com](mailto:Info.ET.Warminster@eurofinsUS.com)